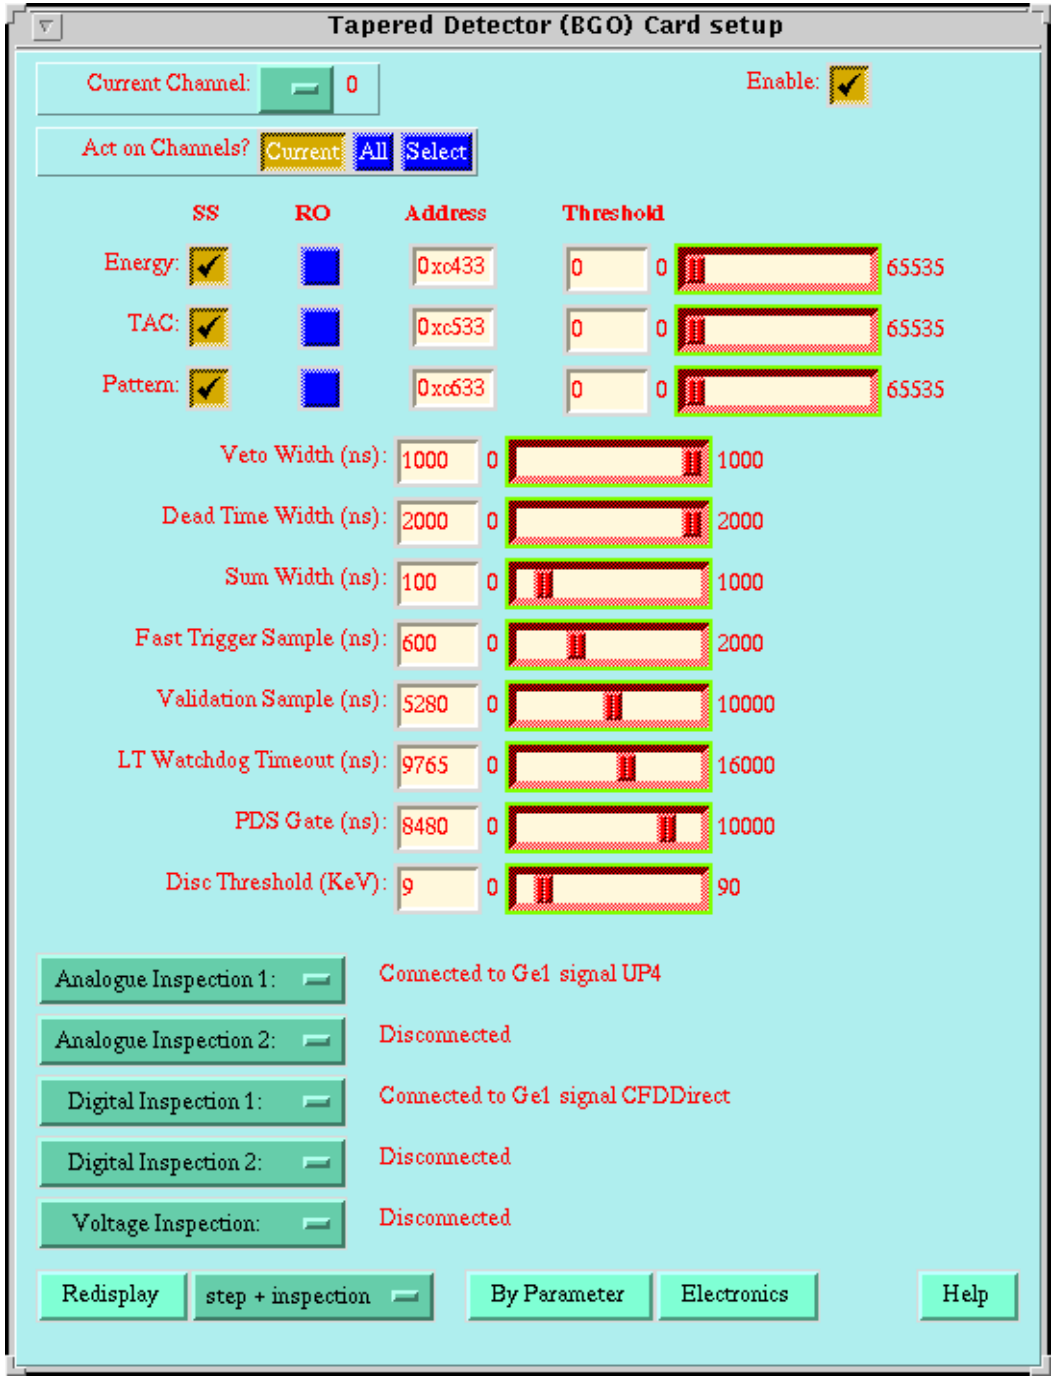
Tapered Detector (BGO) Card setup
Current Channel: 0
Enable:
Act on Channels? Current All Select
SS
RO
Address
Threshold
Energy: 0xc433 0 0 65535
TAC: 0xc533 0 0 65535
Pattern: 0xc633 0 0 65535
Veto Width (ns): 1000 0 1000
Dead Time Width (ns): 2000 0 2000
Sum Width (ns): 100 0 1000
Fast Trigger Sample (ns): 600 0 2000
Validation Sample (ns): 5280 0 10000
LT Watchdog Timeout (ns): 9765 0 16000
PDS Gate (ns): 8480 0 10000
Disc Threshold (KeV): 9 0 90
Analogue Inspection 1: Connected to Ge1 signal UP4
Analogue Inspection 2: Disconnected
Digital Inspection 1: Connected to Ge1 signal CFDDirect
Digital Inspection 2: Disconnected
Voltage Inspection: Disconnected
Redisplay
step + inspection
By Parameter
Electronics
Help